

CONFIRMED
DECEMBER 2007

Non-destructive testing — Magnetic particle testing —

Part 3: Equipment

The European Standard EN ISO 9934-3:2002 has the status of a
British Standard

ICS 19.100

National foreword

This British Standard is the official English language version of EN ISO 9934-3:2002. It is identical with ISO 9934-3:2002

The UK participation in its preparation was entrusted to Technical Committee WEE/46, Non-destructive testing, which has the responsibility to:

- aid enquirers to understand the text;
- present to the responsible international/European committee any enquiries on the interpretation, or proposals for change, and keep the UK interests informed;
- monitor related international and European developments and promulgate them in the UK.

A list of organizations represented on this committee can be obtained on request to its secretary.

Cross-references

The British Standards which implement international or European publications referred to in this document may be found in the BSI Standards Catalogue under the section entitled "International Standards Correspondence Index", or by using the "Find" facility of the BSI Standards Electronic Catalogue.

A British Standard does not purport to include all the necessary provisions of a contract. Users of British Standards are responsible for their correct application.

Compliance with a British Standard does not of itself confer immunity from legal obligations.

This British Standard, having been prepared under the direction of the Engineering Sector Policy and Strategy Committee, was published under the authority of the Standards Policy and Strategy Committee on 30 July 2002

Summary of pages

This document comprises a front cover, an inside front cover, the EN ISO title page, pages 2 to 16, an inside back cover and a back cover.

The BSI copyright date displayed in this document indicates when the document was last issued.

Amendments issued since publication

Amd. No.	Date	Comments

© BSI 30 July 2002

ISBN 0 580 40164 2

English version

**Non-destructive testing - Magnetic particle testing - Part 3:
Equipment (ISO 9934-3:2002)**

Essais non destructifs - Magnétoscopie - Partie 3:
Equipement (ISO 9934-3:2002)

Zerstörungsfreie Prüfung - Magnetpulverprüfung - Teil 3:
Geräte (ISO 9934-3:2002)

This European Standard was approved by CEN on 4 August 2001.

CEN members are bound to comply with the CEN/CENELEC Internal Regulations which stipulate the conditions for giving this European Standard the status of a national standard without any alteration. Up-to-date lists and bibliographical references concerning such national standards may be obtained on application to the Management Centre or to any CEN member.

This European Standard exists in three official versions (English, French, German). A version in any other language made by translation under the responsibility of a CEN member into its own language and notified to the Management Centre has the same status as the official versions.

CEN members are the national standards bodies of Austria, Belgium, Czech Republic, Denmark, Finland, France, Germany, Greece, Iceland, Ireland, Italy, Luxembourg, Malta, Netherlands, Norway, Portugal, Spain, Sweden, Switzerland and United Kingdom.



EUROPEAN COMMITTEE FOR STANDARDIZATION
COMITÉ EUROPÉEN DE NORMALISATION
EUROPÄISCHES KOMITEE FÜR NORMUNG

Management Centre: rue de Stassart, 36 B-1050 Brussels

Contents

Foreword.....	3
1 Scope	4
2 Normative references	4
3 Safety requirements	4
4 Types of devices	4
4.1 Portable electromagnets (AC)	4
4.2 Current generators	6
4.3 Magnetic benches	8
4.4 Specialized testing systems	10
5 UV-A sources.....	11
5.1 Generals.....	11
5.2 Technical data	11
5.3 Minimum requirements	11
6 Detection media system.....	12
6.1 General.....	12
6.2 Technical data	12
6.3 Minimum requirements	12
7 Inspection booth	12
7.1 General.....	12
7.2 Technical data	12
7.3 Minimum requirements	13
8 Demagnetization	13
8.1 General.....	13
8.2 Technical data	13
8.3 Minimum requirements	13
9 Measurements	13
9.1 General.....	13
9.2 Current measurement.....	14
9.3 Magnetic field measurement.....	14
9.4 Visible light measurement	14
9.5 UV-A irradiance measurement.....	15
9.6 Verification and calibration of instruments.....	15
Bibliography	16

Foreword

This document (ISO 9934-3:2002) has been prepared by Technical Committee ISO/TC 135 "Non-destructive testing" in collaboration with Technical Committee CEN/TC 138, "Non-destructive testing", the secretariat of which is held by AFNOR.

This European Standard shall be given the status of a national standard, either by publication of an identical text or by endorsement, at the latest by January 2003, and conflicting national standards shall be withdrawn at the latest by January 2003.

This Standard consists of the following parts :

EN ISO 9934-1	Non destructive testing - Magnetic particle testing - Part 1 : General rules
prEN ISO 9934-2	Non destructive testing - Magnetic particle testing - Part 2 : Detection media
EN ISO 9934-3	Non destructive testing - Magnetic particle testing - Part 3 : Equipment

According to the CEN/CENELEC Internal Regulations, the national standards organizations of the following countries are bound to implement this European Standard: Austria, Belgium, Czech Republic, Denmark, Finland, France, Germany, Greece, Iceland, Ireland, Italy, Luxembourg, Malta, Netherlands, Norway, Portugal, Spain, Sweden, Switzerland and the United Kingdom.

1 Scope

This European Standard describes three types of equipment for magnetic particle testing :

- portable or transportable equipment ;
- fixed installations ;
- specialized testing systems for testing components on a continuous basis, comprising a series of processing stations placed in sequence to form a process line.

Equipment for magnetizing, demagnetizing, illumination, metering and monitoring are also described.

This standard specifies the properties to be provided by the equipment supplier, minimum requirements for application and the method of measuring certain parameters. Where appropriate, measuring and calibration requirements and in-service checks are also specified.

2 Normative references

This European Standard incorporates by dated or undated reference, provisions from other publications. These normative references are cited at the appropriate places in the text and the publications are listed hereafter. For dated references, subsequent amendments to or revisions of any of these publications apply to this European Standard only when incorporated in it by amendment or revision. For undated references the latest edition of the publication referred to applies (including amendments).

EN 10084 *Case hardening steels - Technical delivery conditions*

EN ISO 3059:2001 *Non-destructive testing - Penetrant testing and magnetic particle testing - Viewing conditions (ISO 3059:2001)*

EN ISO 9934-1:2001 *Non-destructive testing - Magnetic particle testing - Part 1 : General rules (ISO 9934-1:2001)*

EN 60529 *Degrees of protection provides by enclosures (IP Code) (IEC 60529:1989)*

3 Safety requirements

The equipment design shall take into account of all European, national and local regulations which include health, safety, electrical and environmental requirements.

4 Types of devices

4.1 Portable electromagnets (AC¹⁾)

4.1.1 General


Hand-held portable electromagnets (yokes) produce a magnetic field between the two poles. (When testing according to EN ISO 9934-1, DC electromagnets should only be used if agreed at enquiry and order stages).

Magnetization shall be determined by measuring the tangential field strength H_t at the centre of a line joining the centres of the pole faces of the electromagnet with pole extenders where used. The electromagnet with a pole spacing s is placed on a steel plate as shown in Figure 1. The plate shall have the dimensions (500 ± 25) mm x (250 ± 13) mm x (10 ± 0.5) mm and shall be of steel conforming to C 22 (EN 10084)..

1) AC = alternative current, and DC = rectified current

Periodic functional checks may be carried out either by the method described above or by a lift test. The electromagnet shall be capable of supporting a steel plate or rectangular bar conforming to C 22 (EN 10084) and having a minimum mass of 4,5 kg, with the magnet poles set at their recommended spacing. The major dimension of the plate or bar shall be greater than the pole spacing s of the electromagnet

NOTE : To lift a steel plate with a mass of 4,5 kg requires a lifting force of 44 N.

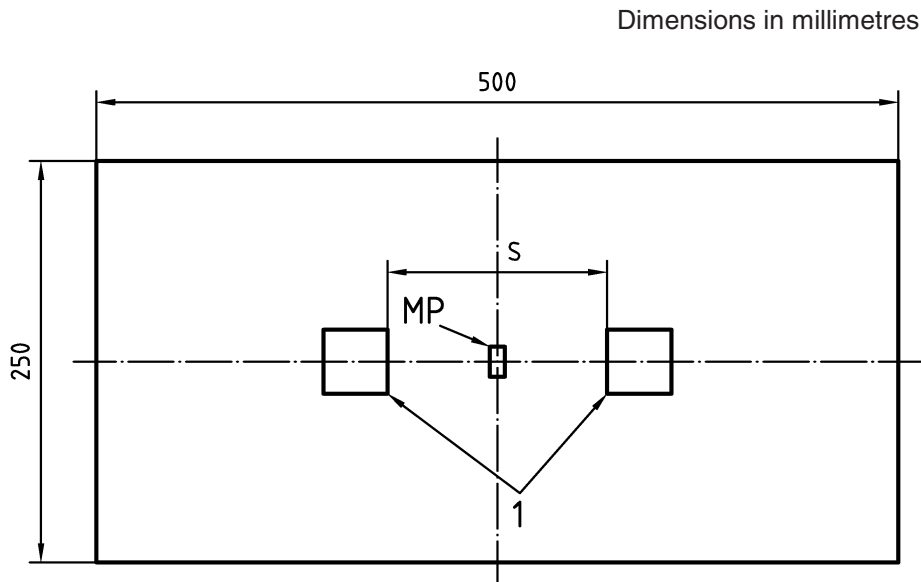

Key

- MP Measuring point for the tangential field strength
- s Pole spacing
- 1 Poles

Figure 1 — Determination of the characteristics of portable electromagnets

4.1.2 Technical data

The following data shall be provided by the equipment supplier:

- recommended pole spacing (maximum and minimum pole spacing) (s_{max} , s_{min});
- cross sectional dimensions of the poles;
- electrical supply (voltage, current and frequency);
- current wave forms available;
- method of current control and effect on waveform (e.g. : thyristor);
- duty cycle at maximum output (ratio of current 'ON' to 'Total' time expressed as a percentage);
- maximum current 'ON' time;
- tangential field strength H_t at s_{max} and s_{min} (following 4.1);
- overall dimensions of the equipment;
- equipment mass, in kilograms;
- specified electrical protection degree (IP) see EN 60529.

4.1.3 Minimum requirements

The following requirements shall be satisfied at an ambient temperature of 30 °C and at maximum output :

- duty cycle $\geq 10 \%$
- current 'ON' time $\geq 5 \text{ s}$
- surface temperature of handle $\leq 40 \text{ °C}$
- tangential field strength at s_{max} (see 4.1) $\geq 2 \text{ kA/m (RMS)}$
- lifting force $\geq 44 \text{ N}$

4.1.4 Additional requirements

The electromagnet shall be supplied with a power ON/OFF switch preferably mounted on the handle.


Generally electromagnets should be usable with one hand.

4.2 Current generators

Current generators are used to supply current for magnetizing equipment. A current generator is characterized by the open circuit voltage U_0 , the short circuit current I_k and the rated current I_r (RMS-values).

The rated current I_r is defined as the maximum current for which the generator is rated at the duty cycle of 10 % and for a current 'ON' time of 5 s if not otherwise specified.

The open circuit voltage U_0 and the short circuit current I_k are derived from the load-characteristic of the generator at maximum power (with any feed back controls disconnected). The load line of the generator may be derived by connecting two widely different loads, such as different lengths of cable, in turn to the generator. For the first cable, the current I_1 through the cable and voltage U_1 across the output terminals are measured and plotted, to give point P_1 on Figure 2. The process is repeated with a second load to give point P_2 . The load line is constructed by drawing a straight line between P_1 and P_2 . The open circuit voltage U_0 and short circuit current I_k are then given by the intercepts on the axes, as shown in Figure 2.

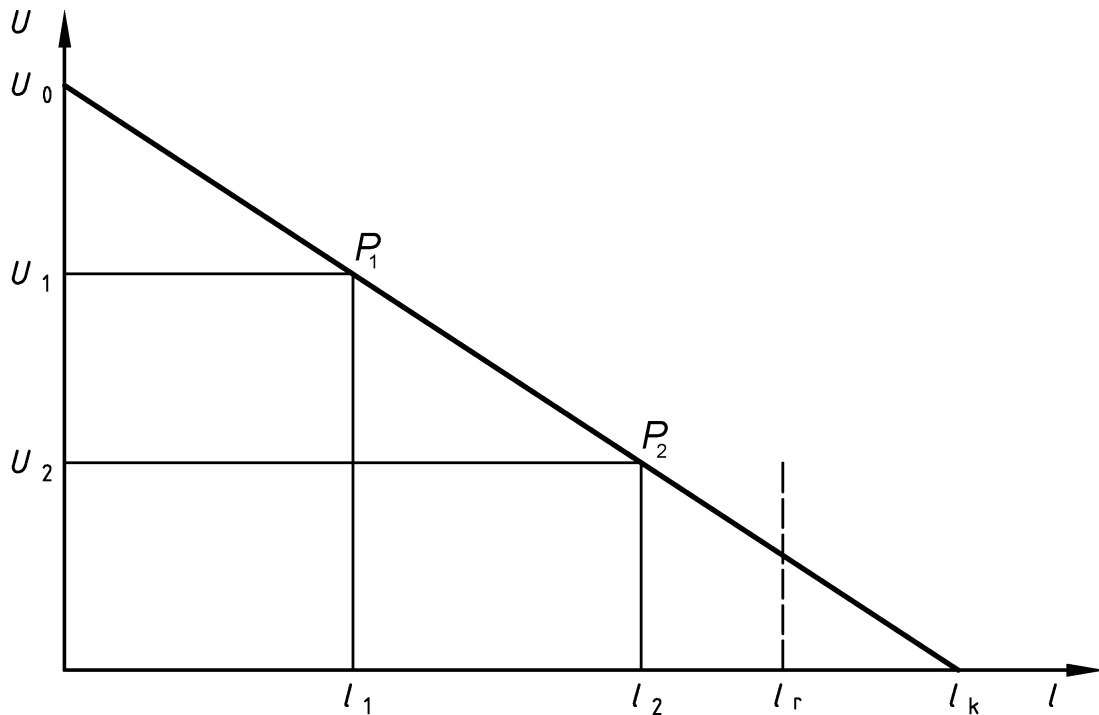

Key

P_1, P_2 Measuring points for determination of the load characteristics

Figure 2 — Load characteristics of the current generator

4.2.1 Technical data

The following data shall be provided by the equipment supplier:

- open circuit voltage U_0 (RMS);
- short circuit current I_k (RMS);
- rated current I_r (RMS);
- duty cycle at maximum output (if other than as specified in 4.2);
- maximum current 'ON' time (if other than specified in 4.2);
- current wave forms available;
- method of current regulation and effect on waveform;
- working range and incremental setting steps;
- method of constant current control if available;
- type of meter (digital, analog);
- resolution and accuracy of current output meter;
- electrical supply requirements at maximum current output (voltage, phases, frequency and current);
- specified electrical protection degree (IP) see EN 60529;

- overall dimensions of equipment;
- equipment mass, in kilograms;
- type of demagnetization if available (see clause 8) .

4.2.2 Minimum requirements

The following minimum requirements shall be satisfied at an ambient temperature of 30°C and at the rated current I_r :

- duty cycle: $\geq 10\%$
- current 'ON' time: $\geq 5\text{ s}$

NOTE : High testing rates will require a higher duty cycle.

4.3 Magnetic benches

4.3.1 General

Fixed installation benches may include facilities for current flow and magnetic flow techniques. Magnetic flow may be achieved either by an electromagnetic yoke or a fixed coil (see EN ISO 9934-1). The characteristics of the current generator are defined in 4.2.

When facilities for multidirectional magnetization are included, each circuit shall be independently controlled. Magnetization shall be sufficient to achieve the required detection capability in all directions.

The characteristic of the electromagnetic yoke is the tangential field strength H_t measured, in kiloamperes per metre, at the midpoint of the length of a cylindrical bar conforming to C22 (EN 10084) of specified dimensions (length and diameter) appropriate to the acceptance range of the equipment.

If the bench is to be used for magnetic flow testing of components longer than 1 m, or segments of the length are magnetized individually, the supplier shall define how magnetizing capability is determined. This shall include a specification of the tangential field strength for a bar of suitable length and diameter.

4.3.2 Technical data

The following data shall be provided by the equipment supplier:

- types of magnetization available;
- current wave forms available;
- method of current control and effect on waveform;
- working range and incremental setting steps;
- method of constant current control if available;
- monitoring of magnetizing current(s);
- magnetizing duration range;
- automated features;
- duty cycle at maximum output;
- maximum current 'ON' time (if other than specified in 4.2);

- tangential field strength H_t (see 4.3);
- open circuit voltage U_0 (RMS);
- short circuit current I_k (RMS);
- rated current I_r (RMS);
- cross sectional dimensions of poles;
- maximum clamping length;
- method of clamping;
- compressed air pressure;
- maximum dimension between headstocks and bed;
- maximum test piece diameter;
- maximum mass of test piece (supported and unsupported);
- type of usable detection media (water-/ oil-based);
- schematic lay out of the equipment (current generator, control panel, location of the detection medium reservoir);
- type of meter (digital, analog);
- accuracy and resolution of meter;
- electrical supply requirements at maximum current output (voltage, phases, frequency and current);
- overall dimensions of equipment;
- equipment mass, in kilograms.
- characteristics of coils:
 - number of turns;
 - maximum achievable ampere turns;
 - length of the coil;
 - internal diameter of the coil or length of sides if the coil is rectangular;
 - field strength in the centre of the coil.

4.3.3 Minimum requirements

The following minimum requirements shall be satisfied at a temperature of 30 °C:

- duty cycle at maximum output $\geq 10 \%$
- current 'ON' time $\geq 5 \text{ s}$
- tangential field strength (see 4.3) $\geq 2 \text{ kA/m}$

— detection capability if required.

4.3.4 Additional requirements

The equipment supplier shall verify the detection capability for a specified component.

4.4 Specialized testing systems

These systems are usually automated and designed for a special task. Complex components may require the use of multidirectional magnetization. The number of circuits and the magnetizing values depend on the location and the directions of the discontinuities to be detected. Therefore in many cases the detection capability can be verified only with test pieces having natural or artificial discontinuities in the relevant zones and directions.

4.4.1 Technical data

The following data shall be provided by the equipment supplier:

- a) number and types of magnetizing circuits;
- b) characteristics of the magnetizing circuits;
- c) current wave forms available;
- d) method of current control and effect on waveform;
- e) working range and incremental setting steps;
- f) method of constant current control if available;
- g) monitoring of the magnetizing current(s);
- h) system cycle time;
- i) prewetting and wetting time;
- j) magnetizing time;
- k) postmagnetizing time;
- l) type of meter (digital, analog);
- m) accuracy and resolution of meter;
- n) duty cycle at maximum output;
- o) maximum current 'ON' time (if other than specified in 4.2);
- p) electrical supply requirements at maximum current output (voltage, phases, frequency and current) ;
- q) type of demagnetization;
- r) type of usable detection media (water-/oil-based);
- s) schematic lay out of the equipment (current generator, control panel, location of the detection medium reservoir);
- t) compressed air pressure;
- u) overall dimensions of equipment;
- v) equipment mass, in kilograms.

4.4.2 Minimum requirements

The following minimum requirements shall be satisfied at a temperature of 30 °C:

- to meet the agreed detection capability;
- to meet the agreed cycle time;
- independent control of each circuit.

5 UV-A sources

5.1 Generals

UV-A sources shall be designed and used in accordance with EN ISO 3059.

5.2 Technical data

The following data shall be provided by the equipment supplier:

- a) surface temperature of the UV-A housing after 1 hour;
- b) type of cooling (e.g. heat exchanger);
- c) electrical supply requirements (voltage, phases, frequency and current);
- d) overall dimensions of equipment;
- e) equipment mass, in kilograms.

At a distance of 400 mm from the UV-A source at the stated voltage:

- f) irradiated area (diameter or length x width measured at half of the maximum surface irradiance);
- g) irradiance after 15 minutes operation;
- h) irradiance after 200 hours continuous operation (typical value);
- i) illuminance after 15 minutes operation (see 9.3);
- j) illuminance after 200 hours continuous operation (typical value).

5.3 Minimum requirements

The following minimum requirements shall be satisfied at a temperature of 30 °C :

- filter resistant against detection media splashes;
- hazard protection of handheld units when in parked position;
- UV-A irradiance at 400 mm from the source $\geq 10 \text{ W/m}^2$;
- illuminance at 400 mm from the source $\leq 20 \text{ lx}$;
- surface temperature of handle $\leq 40 \text{ °C}$.

6 Detection media system

6.1 General

Usually in magnetic benches and specialised testing systems the detection media circulates through the reservoir, wetting units and the drain tray.

6.2 Technical data

The following data shall be provided by the equipment supplier :

- a) agitation method;
- b) material of the reservoir, wetting unit and drain tray;
- c) protection against corrosion;
- d) type of usable detection media (water-/oil-based);
- e) delivery rate of the system;
- f) volume of the reservoir;
- g) electrical supply requirements of the pump, if separate from the equipment;
- h) manual/automated wetting;
- i) fixed/movable wetting unit;
- j) hand hose.

6.3 Minimum requirements

The following minimum requirements shall be satisfied :

- corrosion resistant material for the detection media circuit;
- regulation of the delivery rate.

7 Inspection booth

7.1 General

When using fluorescent detection media, inspection shall be carried out in low ambient visible light to ensure good contrast between discontinuity indications and background (see EN ISO 3059).

For this purpose an inspection booth is required which may be integral with the magnetizing equipment (bench) or it may be a separate free standing enclosure.

7.2 Technical data

The following data shall be provided by the equipment supplier :

- a) visible light in absence of UV-A radiation;
- b) class of flammability;
- c) construction materials;

- d) type of ventilation;
- e) dimensions and access(es).

7.3 Minimum requirements

The following minimum requirements shall be satisfied :

- visible light < 20 lx;
- flame retardant material;
- no glare from visible and/or UV-A radiation within operators field of vision.

8 Demagnetization

8.1 General

Facilities for demagnetization may be included in the magnetizing equipment or, demagnetizing may be carried out using a separate equipment.

If viewing for indications is carried out after demagnetization, indications shall be preserved by a suitable method.

8.2 Technical data

The following data shall be provided by the equipment supplier :

- a) method(s) of demagnetization;
- b) type of current regulation;
- c) field strength (at the centre of the empty demagnetizing coil if applicable);
- d) residual field for a specified component;
- e) electrical supply requirements at maximum current output (voltage, phases, frequency and current) if separate from the general equipment;
- f) overall dimensions of equipment if separate from the general equipment;
- g) equipment mass, in kilograms, if separate from the general equipment.

8.3 Minimum requirements

The equipment shall be capable of demagnetizing to a specified level (typically 0.4 to 1.0 kA/m) unless otherwise agreed

9 Measurements

9.1 General

In connection with this standard, measurements are required for :

- determination of the equipment characteristics;
- checking inspection parameters.

All electric and magnetic values should be specified and measured in RMS values (true). For unidirectional waveforms the RMS-measurement shall take into account the DC-component. If a RMS-measurement is not possible, the measurement method of values shall be declared.

9.2 Current measurement

AC (sinusoidal wave form) can be measured with clamp meters (measuring error < 10 %) or with a shunt and general multipurpose voltage meters (measuring error < 10 %). For measuring phased currents, a meter with a crest factor > 6 (ratio peak value to RMS-value) shall be used.

9.3 Magnetic field measurement

Magnetization may be determined by measuring the tangential field strength using a Hall probe. To obtain the required field strength, three factors should be considered, depending on the method of magnetization and the location of the measurement

a) Orientation of the field-sensitive element

The plane of the field sensitive element should be kept normal to the surface. If a normal field component exists, a tilt may introduce a substantial error.

b) Surface proximity of the field-sensitive element

If the field varies strongly with height above the surface, it may be necessary to make two measurements at different heights to deduce the value at the surface.

c) Direction of the magnetic field

To determine the direction and magnitude of the field, the probe shall be rotated to give the maximum reading.

9.3.1 Technical data

The following data shall be provided by the supplier :

- a) measured value;
- b) type and dimensions of the probe;
- c) distance of the sensor from the probe surface;
- d) geometry of the sensing element;
- e) type of instrument;
- f) dimensions of the instrument;
- g) electrical supply (battery, mains).

9.3.2 Minimum requirements

The following minimum requirement shall be satisfied:

- measurement accuracy better than 10 %.

9.4 Visible light measurement

See EN ISO 3059:2001.

When measuring the visible light from UV sources, the luxmeter shall be insensitive to UV and infrared radiation. Appropriate filters shall be incorporated.

9.5 UV-A irradiance measurement

See EN ISO 3059:2001.

9.6 Verification and calibration of instruments

The verification and calibration procedures for instruments shall be carried out so that during the calibration interval the measuring error remains within limits given in this standard. This shall be done, following the recommendations of the manufacturer of the instrument and in accordance with the quality assurance system of the user.

Bibliography

EN 473 *Qualification and Certification of NDT Personnel - General principles*

EN 1330-1 *Non destructive testing - Terminology – Part 1: General terms*

EN 1330-2 *Non destructive testing - Terminology – Part 2: Terms common to non destructive methods*

prEN ISO 9934-2:2001 *Non-destructive testing - Magnetic particle testing - Part 2 : Detection media*

prEN ISO 12707:2000 *Non destructive testing - Terminology - Terms used in magnetic particle testing*

BSI — British Standards Institution

BSI is the independent national body responsible for preparing British Standards. It presents the UK view on standards in Europe and at the international level. It is incorporated by Royal Charter.

Revisions

British Standards are updated by amendment or revision. Users of British Standards should make sure that they possess the latest amendments or editions.

It is the constant aim of BSI to improve the quality of our products and services. We would be grateful if anyone finding an inaccuracy or ambiguity while using this British Standard would inform the Secretary of the technical committee responsible, the identity of which can be found on the inside front cover. Tel: +44 (0)20 8996 9000. Fax: +44 (0)20 8996 7400.

BSI offers members an individual updating service called PLUS which ensures that subscribers automatically receive the latest editions of standards.

Buying standards

Orders for all BSI, international and foreign standards publications should be addressed to Customer Services. Tel: +44 (0)20 8996 9001. Fax: +44 (0)20 8996 7001. Email: orders@bsi-global.com. Standards are also available from the BSI website at <http://www.bsi-global.com>.

In response to orders for international standards, it is BSI policy to supply the BSI implementation of those that have been published as British Standards, unless otherwise requested.

Information on standards

BSI provides a wide range of information on national, European and international standards through its Library and its Technical Help to Exporters Service. Various BSI electronic information services are also available which give details on all its products and services. Contact the Information Centre. Tel: +44 (0)20 8996 7111. Fax: +44 (0)20 8996 7048. Email: info@bsi-global.com.

Subscribing members of BSI are kept up to date with standards developments and receive substantial discounts on the purchase price of standards. For details of these and other benefits contact Membership Administration. Tel: +44 (0)20 8996 7002. Fax: +44 (0)20 8996 7001. Email: membership@bsi-global.com.

Information regarding online access to British Standards via British Standards Online can be found at <http://www.bsi-global.com/bsonline>.

Further information about BSI is available on the BSI website at <http://www.bsi-global.com>.

Copyright

Copyright subsists in all BSI publications. BSI also holds the copyright, in the UK, of the publications of the international standardization bodies. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI.

This does not preclude the free use, in the course of implementing the standard, of necessary details such as symbols, and size, type or grade designations. If these details are to be used for any other purpose than implementation then the prior written permission of BSI must be obtained.

Details and advice can be obtained from the Copyright & Licensing Manager. Tel: +44 (0)20 8996 7070. Fax: +44 (0)20 8996 7553. Email: copyright@bsi-global.com.

BSI
389 Chiswick High Road
London
W4 4AL